



Non-contact infrared thermometer Instruction manual ST270-01

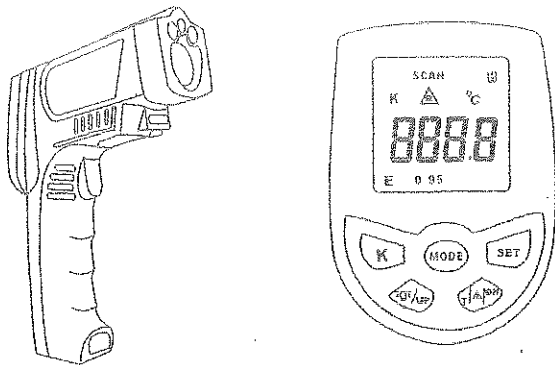

1. Introduction

Compact, rugged and easy to use. Just aim and push the button, read current surface temperatures in less than a second. Safely measure surface temperatures of hot, hazardous or hard-to-reach objects without contact.

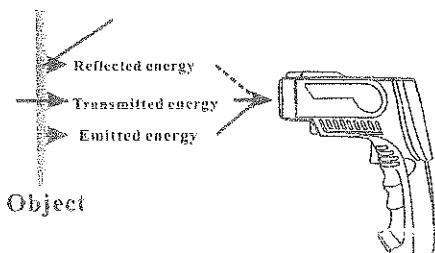


How it works

Infrared thermometer measures the surface temperature of an object. The unit's optics sense emitted, reflected, and transmitted energy which is collect and focused onto a detector. The unit's electronics transmitted energy which is display on the unit. For increased ease and accuracy the laser pointer makes aiming even more precise.

Cautions

Infrared thermometer should be protected for the following:


- EMF(electro-magnetic fields) from arc welders, induction heaters.
- Thermal shock (cause by large or abrupt ambient temperature changes allow 1 hours for unit to stabilize before use).
- Do not leave the unit on or near objects of high temperature.

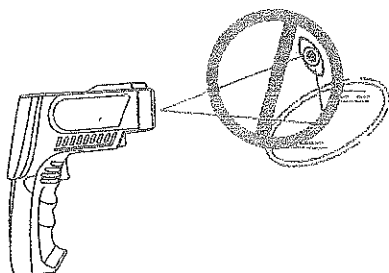

Warning


Do not point laser at eye or indirectly off reflective surfaces.

1. When take measurement, point thermometer toward the object to be measured and hold the yellow trigger. The object under test should be large than the spot size calculated by the field of view diagram.
2. Distance & spot size: As the distance from the object increase, the spot size of measuring area becomes large.

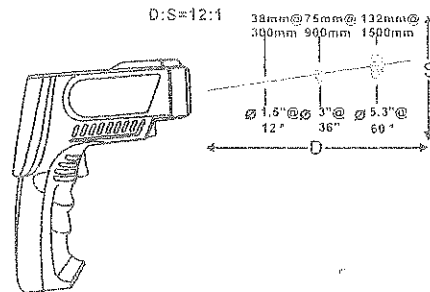


3. Field of view: Make sure the target is larger than the unit's spot size. The smaller the target the close measure distance. When accuracy is critical, make sure the target is at least twice as large as the spot size.
4. Emissivity: Most organic materials and painted or oxidized surfaces have an emissivity of 0.95. Inaccurate readings will result from measuring shiny or polished metal surfaces. To compensate, cover the surface to be measured with masking tape or flat black paint. Measure the tape or painted surface when the tape or painted reach the same temperature as the material underneath

2. Quick start instruction



(Figure1)




(Figure2)

1. Press battery door clip, install battery correctly. Pull the trigger, LCD display reading & battery icon. Release the trigger and the reading will hold for 7 secretary.


LCD display:

- A K type thermocouple working prompt
- B Laser pointer turn on prompt
- C Alarm of high temperature prompt
- D Alarm of Low temperature prompt
- E Data Hold
- F Measure result

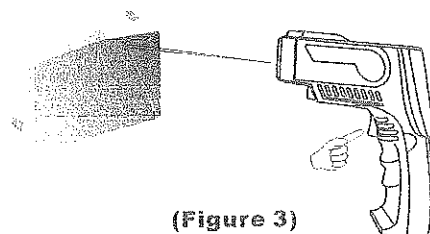


(Figure 3)

2. Locating a hot spot aim the thermometer outside the area of interest, then scan across with up and down motions until you locate the hot spot.(880E model without this function)




(Figure4)



(Figure5)

3. Diagram description

- (1) Trigger : Press for turn on, and then display test result and hold data 7 seconds automatically ("HOLD") after unclamping switch. Trun off automatically after 30 seconds without operate.
- (2) K type thermocouple button : Press for turn on K-type thermocouple measure mode (880E model without K-type function)
Note : As a result of operation principle different , the measure result maybe have a few error of NTC and infrared, it is normal situation.

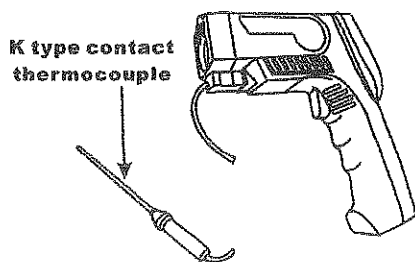

- (3) Back light /Up button : In "Alarm temperature" and "setting emissivity" mode for adjust value up. In other mode for turn on back light. When product working, press it for turn on back light, press again for turn off.
- (4) MODE button: Press MODE button for cycle options - MAX - AVG - MIN -HAL -LAL mode
A、 MAX: Measure maximum data current;
B、 MIN: Measure minimum data current;
C、 AVG: Calculate the average of all measure data;
D、 HAL: Alarm of high temperature. Option HAL mode, press "UP/DN" button for set alarm temperature. When LCD display "H" means measure result exceeded the alarm temperature;
E、 LAL: Alarm of low temperature. Option HAL mode, press "UP/DN" button for set alarm temperature. When LCD display "L" means measure result under the alarm temperature;
- (5) T/ Laser pointer/ DN button : In "Alarm temperature" and "setting emissivity" mode for adjust value down . When turn on product and press direct for °C/°F select.(880E model without Laser pointer function)
- (6) SET button: Press for setting emissivity . And press "UP/DN" for adjust from 0.1~1.0. Press SET button again for exit setting mode.
- (7) LCD

- (8) Battery door: When replace battery door, please using the finger indents to pull open the battery door.

3、 Maintenance

- 1) Lens cleaning: Blow off lose particles using clean compressed air. Gently brush remaining debris away with a moist cotton cloth.
- 2) Case cleaning: Clean the case with a damp sponge/cloth and mild soap.
- 3) Please take out the battery when not using for a long time.

Note:

- 1) Do not use solvent to clean lens.
- 2) Do not submerge the unit in water.

4、 specifications

Temperature range	-30°C to 550°C (-22 to 1022°F)
Accuracy	±2°C or ±2% (Only available for -10°C to 100°C (14 to 212°F) range)
Repeatability	1% of reading or 1°C
Response time	500msec, 95% response
Spectral response	8-14um
Emissivity	0.1~1.0 adjustable
Ambient operating range	0°C to ~40°C (32 to 104°F)
Relative humidity	10-95% RH noncondensing
Storage temperature	-20~60°C (-4~140°F) without battery
Weight/dimensions	130g; 146 × 80 × 38mm
Power	9V Alkaline or NiCd battery
Battery life(alkaline)	Laser models: 12hrs
Display spot size	12:1

Note:

Display "AL" means Ambient temp lower than 0°C";
Display "AH" means Ambient temp higher than 60°C";
Display above code in normal Ambient temp, probable means this meter was broken.

Attached list : Applicable Emissivity for Different Material (For reference only)

Material	Emissivity	Material	Emissivity
Asphaltum	0.90 to 0.98	Textile (Black)	0.98
Beton	0.94	Human Skin	0.98
Cement	0.96	Soap bubble	0.75 to 0.80
Sand	0.90	Charcoal (powder)	0.96
Soil	0.92 to 0.96	Lacquer	0.80-0.95
Water	0.92 to 0.96	Lacquer (reluster)	0.97
Ice	0.96 to 0.98	Rubber (Black)	0.94
Snow	0.83	Plastic	0.85-0.95
Glass	0.90 to 0.95	Timber	0.90
Ceramic	0.90 to 0.94	Paper	0.70-0.94
Marble	0.94	Chromic oxide	0.81
Gypsum	0.80 to 0.90	Copper Oxide	0.78
Compo	0.89 to 0.91	Iron Oxide	0.78 to 0.82
Brick	0.93 to 0.96	Stainless steel	0.2-0.3